

FIG. 1B





FIG. 2

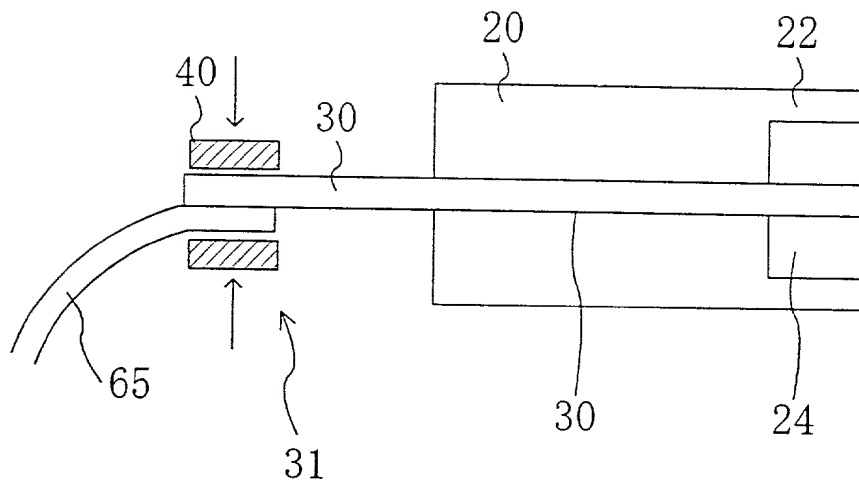

3/8

FIG. 3


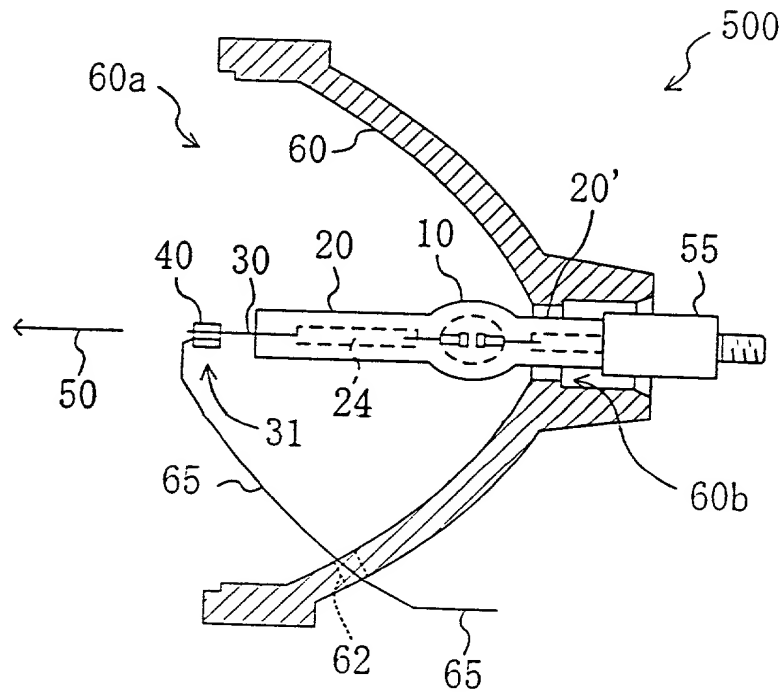


FIG. 4

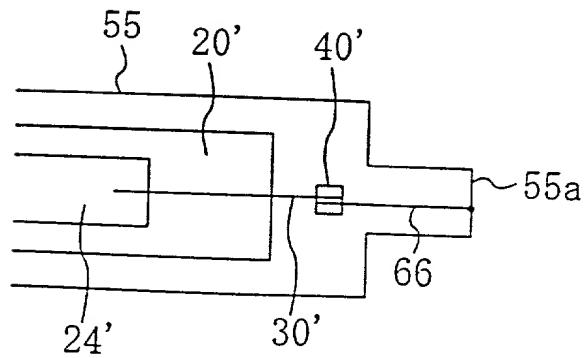

4/8

FIG. 5

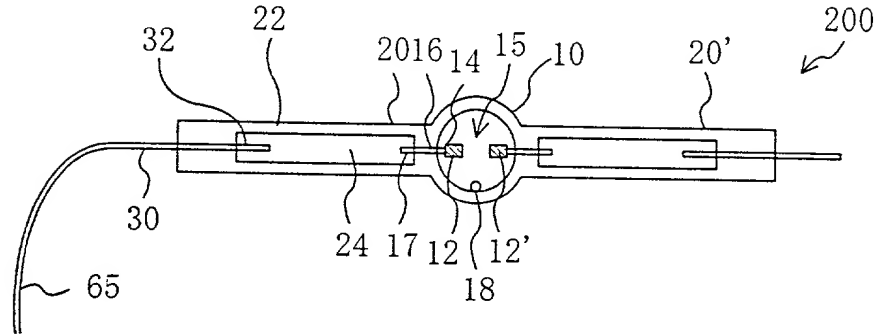


FIG. 6

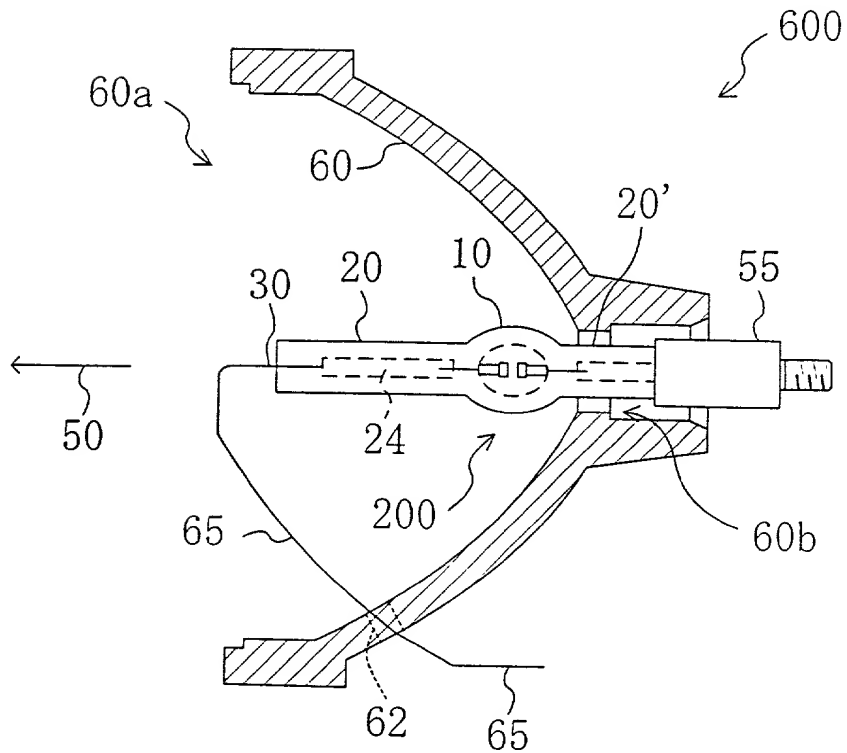


FIG. 5

A cross-sectional view of a medical device 100 inserted into a body cavity 30. The device 100 includes a handle 60, a shaft 64, and a distal tip 62. The distal tip 62 is positioned within the cavity 30. A dashed line 65 indicates the position of the distal tip 62 when the device is retracted.

6/8

FIG. 8A

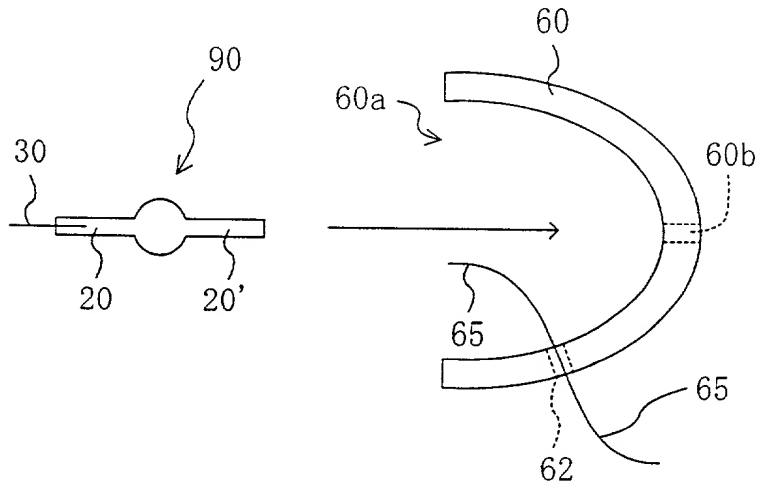


FIG. 8B


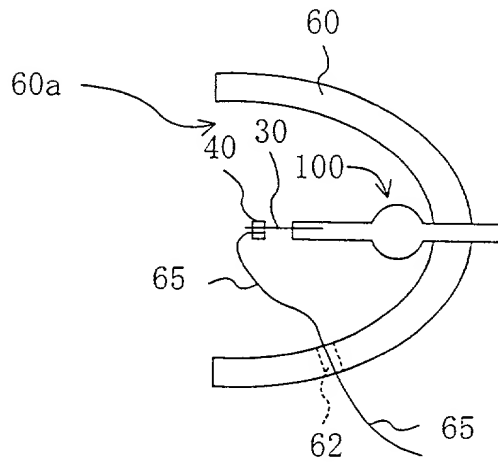


FIG. 8C

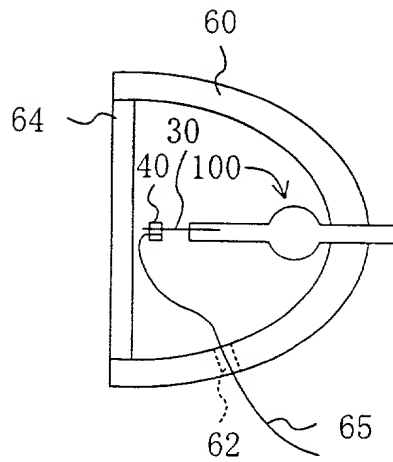

7/8

FIG. 9

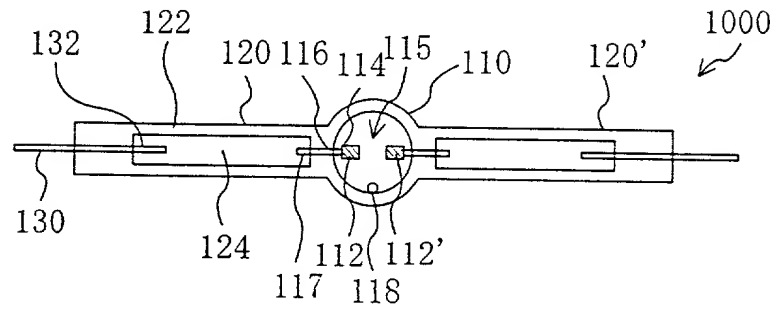


FIG. 10

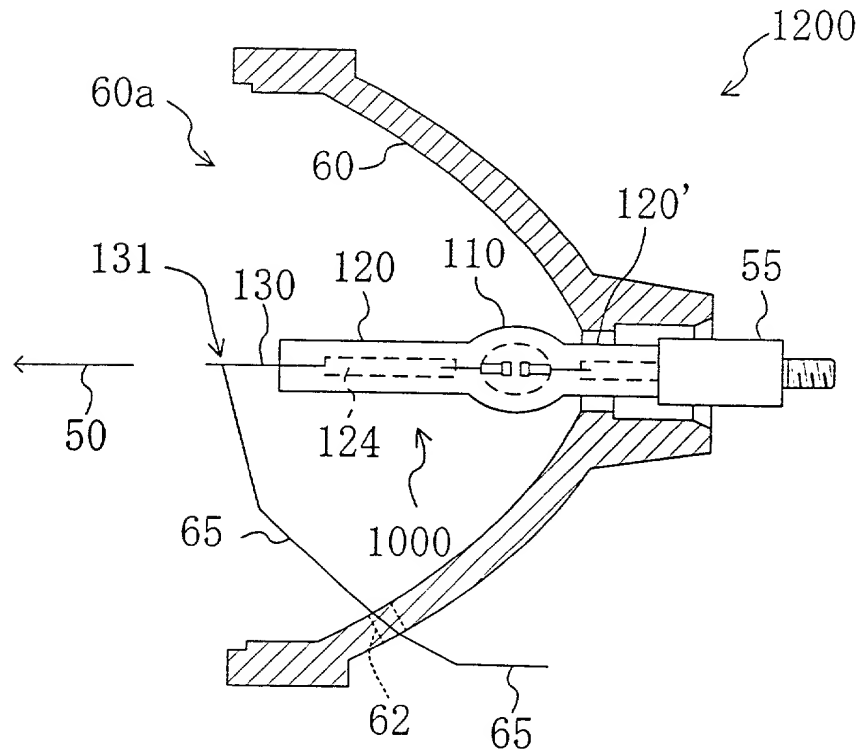


FIG. 11

